

H117 Stage

Motorized Precision Stage for Inverted Microscopes

The H117 is a precise, reliable and repeatable stage ideal for a wide range of applications and compatible with a vast range of inverted microscopes. Controlled via Prior's ProScan® III system, the H117 offers the end user the specifications needed to achieve exceptionally high quality imaging. By automating the microscope stage, the end user increases the speed of image collection, can accurately image exact regions of the sample, and program in specific stage movements. Stage automation also significantly decreases the risk of fatigue, strain injuries, and operator error.

Precise:

- ± 0.2 μm mean uni-directional repeatability
- 0.059 µm/mm average metric accuracy
- 0.01 μm resolution
- Intelligent Scanning Technology (IST) increases accuracy of movement
- Anti-backlash mechanism as standard
- Linear encoders can be added to further increase accuracy



Versatile:


- Large, flat top surface area and travel range (114 x 75 mm)
- Suggested maximum speed of 15 mm/s
- Limit switches allow stage movement to be constrained if required to avoid collisions
- Fits to almost all common inverted microscopes from Nikon, Olympus, Zeiss and Leica
- Control via ProScan® III means stage can be controlled by almost any commercial available imaging software package





COMPATIBLE WITH:


- Olympus IX73/83 series microscopes
- Olympus IX71/81 series microscopes
- Nikon Ti and Ti2 series microscopes
- Nikon MA200 series microscopes
- Zeiss Axiovert series microscopes
- Zeiss AxioObserver series microscopes
- Leica DMI 3000, 4000, 5000 and 6000B series microscopes
- Leica DMi8 series microscopes
- Prior FB series focus blocks
- Contact Prior for information on non-standard applications we might still be able to mount it!


Motorized Precision Stage for Inverted Microscopes



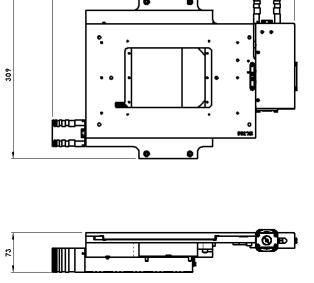

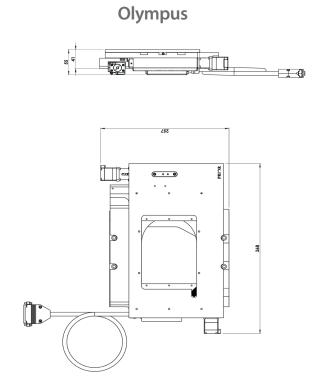

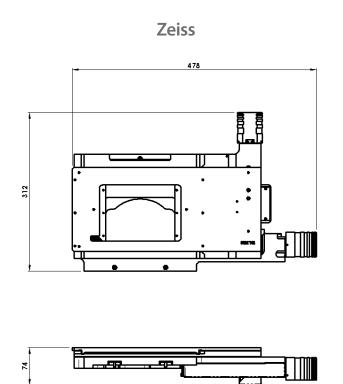

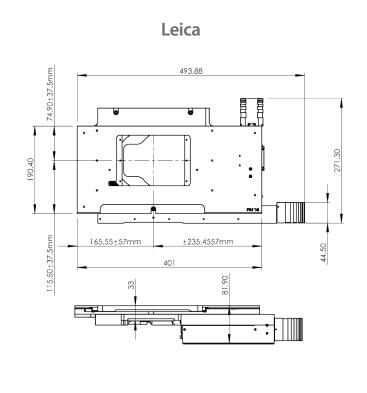

H117

Motorized Precision Stage for Inverted Microscopes



SPECIFICATIONS

| PART NUMBER | H117P1## | H117E1## | Note that these specifications were obtained via the Prior method of testing using a Prior controller. | |
|--|----------|----------|--|--|
| Mean uni-directional repeatability* (μm) | 0.2 | 0.2 | method of testing using a Prior controller. | |
| Resolution (µm) | 0.01 | 0.01 | A # indicates at what point the microscope code should be | |
| Suggested max speed (mm/s) | 15 | 15 | inserted; e.g. H117E1NN or H117P1N4. Note that other stages | |
| Average metric accuracy** (µm/mm) | 0.059 | 0.046 | are also available - contact Prior scientific for more information. | |
| Maximum travel range (mm) | 114 x 75 | 114 x 75 | | |
| Maximum load (kg) | 10 | 10 | *Based on performance with the IST enabled measured over the | |
| Squareness (arc seconds) | 30 | 30 | full range of travel. | |
| Ball screw pitch (mm) | 1 | 1 | **Using a Prior ProScan controller with backlash correction | |
| Motor type (SPR***) | 400 | 400 | enabled; all repeatability is uni directional. | |
| Encoders | no | Yes | ***Steps per Revolution of Motor | |

ORDERING INFORMATION

| MICROSCOPE | H117 STAGE | ENCODED H117 STAGE |
|------------------------|------------|--------------------|
| Olympus IX71/73/83 | H117P1XD | H117E1XD |
| Olympus IX81 | H117P1I4 | H117E1I4 |
| Nikon MA200 | H117N1M4 | H117E1M4 |
| Nikon Ti/Ti2 | H117P1NN | H117E1NN |
| Zeiss Axiovert | H117P1X4 | H117E1X4 |
| Zeiss AxioObserver | H117P1X4 | H117EIX4 |
| Leica DMI /DMi8 series | H117P1D4 | H117E1D4 |

Please contact Prior Scientific before ordering and confirm the microscope before placing an order.

This is not an exhaustive list, please contact Prior if you have a rarer or non standard microscope, or do not wish to mount the H117 on a microscope.

WORLDWIDE DISTRIBUTION

Prior Scientific Ltd 3-4 Fielding Industri Estate, Wilbraham Road, Fulbourn, Cambridge, CB21 5ET, UK

Prior Scientific 80 Reservoir Park Drive Hans-Knöll-Str. 6 Rockland, MA 02370 **USA**

D-07745 Jena, Germany

Prior Scientific GmbH Prior Scientific KK Kayabacho 3rd Nagaoka Prior Scientific Bldg 10F, 2-7-10, Nihonbashi Kayabacho, Chuo-Ku, Tokyo, 103-0025, Japan

Prior Scientific China Instruments (Suzhou) Ltd. 509 Tayun Plaza, 188 Tayun Road Suzhou, 215000 China

